

## Cautions about using Input Modules

The following items should be strictly obeyed for the safe usage of these products, and for protecting yourself and other people from bodily harm and/or damage to property. Before using any of these products, please read the following carefully and fully understand the contents.

- Do not connect any of the Input Modules in this manual to any Data Logger other than RTR-505 / TR-55i.
- Do not take apart, repair or modify an Input Module.
- Use Input Modules only in an environment where the ambient temperature is from -40 to 80°C and the humidity is 90%RH (no condensation) or less.
- For information about handling sensors and their necessary operating environments, see the User's Manual included with the sensor.
- Do not use or store Input Modules in places such as listed below. It may result in malfunction or unexpected accidents.
  - Areas exposed to direct sunlight
  - In water or areas exposed to water
  - Areas exposed to organic solvents and corrosive gas
  - Areas exposed to strong magnetic fields
  - Areas exposed to static electricity
  - Areas near fire or exposed to excessive heat
  - Areas exposed to excessive dust or smoke
- The sensor connection of Input Modules is not water resistant; make sure not to get wet.
- Do not use alcohol to clean Input Modules. If an Input Module gets dirty, wipe it with a soft cloth dipped in water and tightly wrung out.
- Do not drop or expose an Input Module to a strong impact.
- Do not use an Input Module on the human body.
- Store Input Modules out of the reach of children.
- If any smoke, strange smells or sounds are emitted from an Input Module, immediately stop using.
- When making "Adjustment Settings" using the software, the adjustment values will be saved to the Input Module. Therefore, when an Input Module is replaced, it is necessary to re-make any desired adjustment settings to be written into the newly connected module.

## Input Module User's Manual

Carefully read this instruction manual before using any of these products.

### Thermocouple Module (TCM-3010)

### PT Module (PTM-3010)

### Voltage Module (VIM-3010)

### 4-20mA Module (AIM-3010)

### Pulse Input Cable (PIC-3150)

In this manual, the modules listed above are collectively referred to as (an / the) "Input Module(s)" and RTR-505 / TR-55i as the "Data Logger".

Distributed by MicroDAQ.com, Ltd.  
[www.MicroDAQ.com](http://www.MicroDAQ.com)  
 (603) 746-5524

## T&D Corporation

<http://www.tandd.com/>


817-1 Shimadachi Matsumoto, Nagano 390-0852 JAPAN

Fax:+81-263-40-3152

© Copyright T&D Corporation. All rights reserved.  
 This is printed using recycled paper.

2012.03 16504750004 (1st Edition)

## Thermocouple Module (TCM-3010)

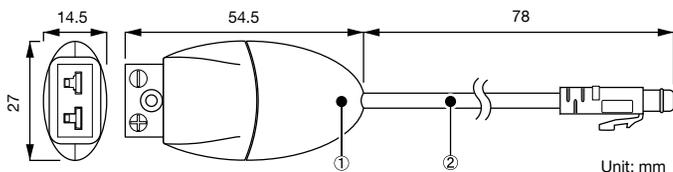

Materials: ① Polycarbonate ② Vinyl Coated Electrical Wire


Measurement Item	Temperature	
Compatible Sensors	Thermocouple: Type K, J, T, S	
Measurement Range	-199 to 1700°C (only within the sensor heat-durability range)	
Measurement Resolution	Type K, J, T : 0.1°C Type S : about 0.2°C	
Measurement Accuracy*	Thermocouple Measurement	±0.3°C + 0.3% of reading (Type K, J, T) ±1°C + 0.3% of reading (Type S)
	Cold Junction Compensation	±0.3°C (10 to 40°C), ±0.5°C (-40 to 10°C / 40 to 80°C) The above mentioned temperature is the operating environment for Input Module only.
Sensor Connection	Miniature Thermocouple Connector	
Operating Environment	Temperature: -40 to 80°C, Humidity: 90%RH or less (no condensation)	

\* Sensor error is not included.

### CAUTION


- When inserting a sensor into an Input Module, ensure that the polarity is correct by aligning the plus and minus signs on the sensor connector and the module.
- The Data Logger detects the break of wire every 40 seconds or so, causing it to display an uncertain temperature directly after a connector is removed.
- After connecting an Input Module to a Data Logger, check the thermocouple type (K, J, T, or S) of the sensor to be used and the sensor type to be displayed on the LCD screen of the Data Logger; make sure they are the same. If they are different, change the sensor type using the software.
- Measurement range is in no way a guarantee of the sensor heat-durability range. Check and confirm the heat durability of the sensor.
- When the sensor is broken or unconnected, the message "Err" will appear on the LCD screen of the Data Logger.

### Connecting the Sensor



1. Check the sensor type and the polarity (plus and minus signs).
2. Insert the sensor connector, aligning as shown on the Input Module.

## PT Module (PTM-3010)

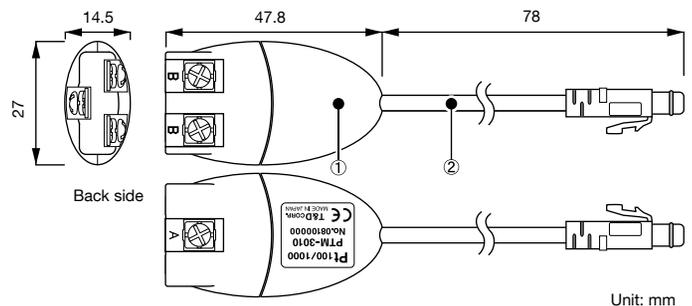

Materials: ① Polycarbonate ② Vinyl Coated Electrical Wire

Measurement Item	Temperature
Compatible Sensors	Pt100 (3-wire), Pt1000 (3-wire)
Measurement Range	-199 to 600°C (only within the sensor heat-durability range)
Measurement Resolution	0.1°C
Measurement Accuracy*	±0.3°C + 0.3% of reading (10 to 40°C), ±0.5°C + 0.3% of reading (-40 to 10°C / 40 to 80°C)
	The above mentioned temperature is the operating environment for Input Module only.
Sensor Connection	Screw Clamp Terminal Block (3-Terminal)
Operating Environment	Temperature: -40 to 80°C, Humidity: 90%RH or less (no condensation)
Accessories	Protection Cover

\* Sensor error is not included.


### CAUTION

- After connecting an Input Module to a Data Logger, check the type (100Ω or 1000Ω) of the sensor to be used and the sensor type to be displayed on the LCD screen of the Data Logger; make sure that they are the same. If they are different, change the sensor type using the software.
- Make sure to correctly connect the lead wires according to the diagram shown on the terminal block, and securely tighten the screws to the terminal block.
- The two "B" terminals have no polarity.
- Measurement range is in no way a guarantee of the sensor heat-durability range. Check and confirm the heat durability of the sensor.
- When the sensor is broken or unconnected, the message "Err" will appear on the LCD screen of the Data Logger.

### Connecting the Sensor

1. Loosen the screws of the terminal block.
2. Remove the protection cover from the Input Module, and place it through the sensor cable.
3. Insert terminals A and B according to the diagram shown on the terminal block.
4. Firmly tighten the screws to the terminal block.
5. Replace the protection cover over the terminal block.

## Voltage Module (VIM-3010)

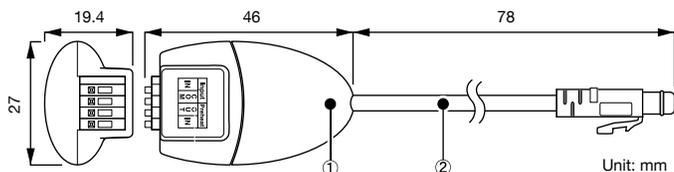

Materials: ① Polycarbonate ② Vinyl Coated Electrical Wire


Measurement Item	Voltage
Input Voltage Range	0 to 999.9mV, 0 to 22V Breakdown voltage: $\pm 28V$
Measurement Resolution	up to 400mV: at 0.1mV, up to 800mV: at 0.2mV, up to 999mV: at 0.4mV, up to 3.2V: at 1mV, up to 6.5V: at 2mV, up to 9.999V: at 4mV, up to 22V: at 10mV
Measurement Accuracy	$\pm 0.5\text{ mV} + 0.3\%$ of reading (10 to 40 °C), $\pm 1\text{ mV} + 0.5\%$ of reading (-40 to 10 °C / 40 to 80 °C) The above mentioned temperature is the operating environment for Input Module only.
Input Impedance	mV Range: About 3M $\Omega$ , V Range: About 1M $\Omega$
Preheat Function	Voltage Range (Preheating): 3V to 20V/100mA, Time Range (Preheating): 1 to 999 seconds (in units of one-second) Diode for backflow prevention built in the "Preheat OUT" side
Sensor Connection	Cable Insertion Connection: 4-Terminal
Compatible Wires	Single wire: $\phi 0.32$ to $\phi 0.65\text{mm}$ (AWG28 to AWG22), $\phi 0.65\text{mm}$ (AWG22) recommended Twisted wire: 0.32mm <sup>2</sup> (AWG22), $\phi 0.12\text{mm}$ or more in diameter Strip length: 9 to 10mm
Operating Environment	Temperature: -40 to 80°C / Humidity: 90%RH or less (no condensation)

### CAUTION

- It is not possible to measure negative voltage with this module.
- When the signal source output impedance is high, a gain error will occur due to the change in input impedance.
- For details about the preheat function, see the User's Manual that comes with the software or the Help Menu in the software you are using.
- Voltage to be input to "Preheat" should be 20V or lower. Inputting a higher voltage may cause damage to the Input Module.
- When the preheat function is not being used, do not connect anything to the "Preheat IN" or "Preheat OUT".
- When using the preheat function, output signal GND(-) and power GND(-) need to be connected together.
- The LCD refresh interval for the Data Logger is basically from 1 to 10 seconds, but when using the preheat function the LCD display will be refreshed based on the recording interval set in the Data Logger.
- When you remove the lead wires from the Input Module, core wires will be exposed; be careful of electric shock or short circuits.


### Connecting the Sensor

- Using a screwdriver or tweezers, while pressing down on the terminal button, insert the wire into the hole.




- Also when removing, gently pull the wire out of the hole while pressing down on the terminal button.

### Example of Sensor Connection



## 4-20mA Module (AIM-3010)

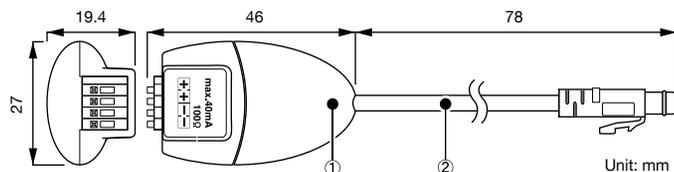

Materials: ① Polycarbonate ② Vinyl Coated Electrical Wire


Measurement Item	4-20mA
Input Current Range	0 to 20mA (Operational up to 40mA)
Measurement Resolution	0.01mA
Measurement Accuracy	$\pm 0.05\text{ mA} + 0.3\%$ of reading (10 to 40 °C), $\pm 0.1\text{ mA} + 0.3\%$ of reading (-40 to 10 °C / 40 to 80 °C) The above mentioned temperature is the operating environment for Input Module only.
Input Resistance	100 $\Omega \pm 0.3\Omega$
Sensor Connection	Cable Insertion Connection: Plus(+) 2 Parallel Terminals, Minus(-) 2 Parallel Terminals: Total 4 Terminals
Compatible Wires	Single wire: $\phi 0.32$ to $\phi 0.65\text{mm}$ (AWG28 to AWG22), $\phi 0.65\text{mm}$ (AWG22) recommended Twisted wire: 0.32mm <sup>2</sup> (AWG22), $\phi 0.12\text{mm}$ or more in diameter Strip length: 9 to 10mm
Operating Environment	Temperature: -40 to 80°C / Humidity: 90%RH or less (no condensation)

### CAUTION

- Do not apply electric current exceeding the input current range. Doing so may damage the Input Module, causing heat or fire to occur.

### Connecting the Sensor


- Using a screwdriver or tweezers, while pressing down on the terminal button, insert the wire into the hole.




- Also when removing, gently pull the wire out of the hole while pressing down on the terminal button.

### Example of Sensor Connection

It is possible to connect a sensor and a voltage meter to the module at the same time.



## Pulse Input Cable (PIC-3150)

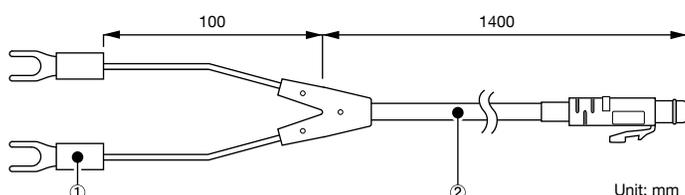

Materials: ① M3.5 Crimp Terminal ② Vinyl Coated Electrical Wire

Measurement Item	Pulse Count
Input Signal	Non-voltage Contact Input / Voltage Input (0 to 27 V) Breakdown voltage: -5V, +27V
Detection Voltage	Lo: 0.5V or less, Hi: 2.5V or more
Chattering Filter	ON (15Hz or less) / OFF (3.5kHz or less) 0-3V Rectangular Wave Signal
High Level Pulse Width	Chattering Filter ON: 35ms or more, Chattering Filter OFF: 180 $\mu\text{s}$ or more
Low Level Pulse Width	Chattering Filter ON: 12ms or more, Chattering Filter OFF: 100 $\mu\text{s}$ or more
Response Polarity	Select either Lo->Hi or Hi->Lo
Maximum Count	61439 / Recording Interval
Input Impedance	Approx. 100k $\Omega$ pull up
Max Jitter	Normal: About 0.01 seconds, During Communication: About 0.1 seconds

### CAUTION

- Note that the specifications listed above are for the RTR-505 / TR-55i being connected to this pulse input cable.
- When connecting the cable to the measurement object, make sure to check the terminal polarity (RD: +, BK: -) in order to wire properly.

Distributed by MicroDAQ.com, Ltd.  
www.MicroDAQ.com  
(603) 746-5524